

#2064

**CSIRO
Division of Building Research
P.O. Box 56
Highett, Victoria 3190
AUSTRALIA**

© CSIRO, 1983

ISBN 0 643 03588 5

Printed by BUILDRESEARCH Melbourne

OUTLINE OF AN APPARATUS FOR CONTINUOUS MONITORING OF AIR INFILTRATION IN HOUSES

SUMMARY

Air infiltration, defined as uncontrolled leakage of air through the building envelope, affects the heating and cooling loads of houses, and the quality of air within them. Its magnitude is therefore of considerable importance. Continuous monitoring is an efficient method for obtaining the large amount of air infiltration rate data needed to characterize the infiltration behaviour of a house.

The principle of a method for continuous monitoring of air infiltration rate is explained and an outline given of an apparatus to implement it. The apparatus consists of an infra-red gas analyser with six air sampling tubes and a rotating multi-port gas valve; a gas distribution system comprising a gas cylinder, a gasometer, a flowmeter with needle valve, and six solenoid-operated gas valves; electronic control circuitry; a data logger and printer; meteorological instrumentation; and a multi-channel chart recorder.

The sequence of operations of the apparatus, the tracer gas distribution system, and the calculation of infiltration rates are discussed. An expression is given linking the maximum values of infiltration rate and building volume that may be monitored by the apparatus as it is presently adjusted.

Keywords: Infiltration, Continuous measurement, Constant concentration, Apparatus.

1. INTRODUCTION

Ventilation of buildings is essential in order to meet the oxygen requirements of the occupants and to keep the concentration of carbon dioxide sufficiently low. It also enables the control of factors such as tobacco smoke, odours, humidity, and indoor pollution arising from materials used in furniture, furnishings, and house construction.

Energy required in buildings to provide thermal comfort and hot water, and for cooking, lighting and the operation of appliances, accounts for more than 20% of Australia's primary energy consumption (National Energy Advisory Committee, 1980). About two-thirds of this energy is used in domestic buildings and in south-eastern Australia almost half the domestic energy usage is accounted for by space heating. Energy must be consumed to heat the air entering a house maintained above ambient temperature. Depending upon the extent to which the house is thermally insulated, this energy consumption can account for as much as 40 per cent of the total heating load. There is, therefore, a strong incentive to reduce air infiltration in houses. (Air infiltration may be defined as

uncontrolled leakage of air through cracks and openings in the building envelope).

From either point of view, i.e. the provision of an adequate supply of air for health and comfort, or the restriction of air infiltration in order to reduce energy consumption, it is of basic importance to be able to measure the infiltration rate. Known values are necessary, too, for accurate calculations of heating loads.

The infiltration rate for a given building is dependent on, among other things, the speed and direction of the wind to which it is exposed, and on the temperature difference between indoors and outdoors. Thus to characterize the infiltration behaviour of a building, values of infiltration rate will be required for a range of wind speeds and directions, and a range of indoor to outdoor temperature differences. The data can be obtained efficiently by continuous, automatic monitoring.

The basic principles of measuring the rate of air infiltration into buildings by means of a tracer gas have been described by many authors including Kronvall (1980) and Grot *et al.* (1982), and a number of measuring

relation $T = 90t$. This has been done for reference concentrations of 70 and 99 ppm, six gas sample and release locations, with fifteen gas releases per hour at each location ($q = 11.6 \text{ mL/s}$), with a house volume of 250 m^3 , and the results are shown in Figure 1.

It may be seen from Figure 1 that the calculated air infiltration rate, γ , increases non-linearly with T , the total time of gas release per hour, and that for a given value of γ the magnitude of T increases with the reference concentration C_R . The latter has practical implications. If the air infiltration rate of the house is low the value of T obtained by measurement will be low and the value of t , the number of seconds of gas released on each occasion, at each location, will be small, leading to possible inaccuracies. Thus C_R should be set at a relatively high value. On the other hand, if the air infiltration rate is high the value of t required to establish a stable concentration may exceed the time available for gas release on each occasion, so C_R should be set at a relatively low figure.

A block diagram of the apparatus is shown in Figure 2. The sequence of operations, which is controlled by the cycle control unit, is depicted in Figure 3. In outline, the sequence of events is to sample gas at position 1, compare the measured concentration C_M with the reference concentration C_R and use the difference in concentration [$C_R - C_M$] to control the time of release of gas by means of the gas release unit acting on the gas distribution unit, which in turn releases the gas at location 1 in the general vicinity of that sampling point. A domestic exhaust fan with a capacity of $580 \text{ m}^3/\text{h}$, mounted near the floor (see Fig. 4) is used at each location to ensure dispersal of the gas and thorough mixing with the air. Before moving to position 2 the printer records the sample location, the time of day, gas concentration and the accumulated total number of seconds during which gas has been released. This sequence of operations is repeated for locations 2 to 6, followed by the recording of temperature and wind data. The time taken to complete one cycle of operations is set, by means of an adjustable delay at the beginning of the cycle, to be 4 minutes precisely, which ensures that there are fifteen releases of gas per hour at each location.

In addition to the printout, a multi-channel chart recorder provides traces of the indoor and outdoor temperatures, the wind speed averaged over two minutes, wind direction sampled at one minute intervals, and by means of a suitable circuit, the gas concentration at each of the six locations is sampled sequentially and each concentration recorded for approximately 30 seconds on a single trace. A sample of the chart recording is shown in Figure 5. This chart is particularly useful as a guide to the selection of times suitable for the processing of the air infiltration data; that is, when the weather conditions are stable and infiltration rates are within the range that can be measured with the apparatus (this latter aspect is discussed at the end of the next section).

3. SOME DETAILS OF THE APPARATUS

The concentration of tracer gas at a given location is determined by drawing a stream of the tracer gas/air mixture from that location by means of an inbuilt diaphragm pump, operating at approximately 1 L/min. , and passing it through a gas analyser which utilizes a double-beam system employing a gas-filled detector operating in the infra-red region at wavelengths between 2 and $15 \text{ }\mu\text{m}$. There it is compared with tracer-free air drawn from outside the building being tested. The particular location sampled is determined by the position of a multi-port, step-rotating gas port selector (Scanivalve Type S1265-1P/12T) which is under the direction of the cycle control unit. A separate pump, operating at about 17 L/min. , maintains a flow of air through all the sampling tubes not coupled to the gas analyser at that time, in order to reduce the time to reach equilibrium when the gas valve is rotated to select the next location to be sampled. (Thirty seconds has been allowed for equilibration). The flowrates are low and have negligible effect on the distribution of tracer gas within the volume under consideration and on the air infiltration rates being determined.

At each of the six locations, tracer gas is released, via a solenoid-operated valve, on the inlet side of a fan mounted near the floor and directing its air stream vertically upwards, to ensure good mixing with the room air. (Smoke pencil tests have shown that all parts of a room are involved in the mixing process. Furthermore, four minutes elapses between the release of gas at a given location and the next sampling of the gas concentration there). For each location the number of seconds during which gas is released is added to the total number of seconds of gas release for the whole house being accumulated in a counter.

It is a requirement of this method for determining air infiltration rates that gas is released at a constant flowrate. Figure 6 shows the essential features of the gas distribution system designed to achieve this. An inverted, weighted, hollow cylinder 140 mm in diameter and 240 mm high, closed at the top, located in an outer, open-topped hollow cylinder partly filled with transformer oil, is used as a storage tank in a manner similar to a 'gasometer'. The storage tank is 'charged' by gas entering it from the N_2O cylinder via regulating valves and the solenoid-controlled gas valve. Intervals for charging (or 'topping up') are provided six times per cycle, as indicated in Figure 3, so that the storage tank is normally at or near its full capacity at the start of each period of gas release. The gasometer is shown in Figure 7. (Nitrous oxide is only sparingly soluble in the oil used and, within the limits of experimental error, no difference has been detected between infiltration rates obtained with the gasometer open to the room and those obtained with the gasometer in a gas-tight enclosure).

As a check on the performance of the automatic apparatus, the release of tracer gas was stopped on several occasions, in different houses, and the decay in concentration of tracer gas measured over time periods of up to several hours. The air change rate was determined for periods during the decay of approximately one hour, from the expression

$$\gamma = [\ln C_0 - \ln C_1] / H$$

where C_0 is the initial gas concentration (ppm),

C_1 is the final gas concentration,

and H is the time for the decay (hours).

The values for the air change rates obtained by this method were within 10% of those using the automated gas release method for the same nominal wind velocity and approximate wind direction. This is considered good agreement since the wind conditions always changed to some extent over the comparison period and the air change rate is dependent on the precise wind speed and direction.

The equipment described here does not employ micro-processor technology, but the principle of the method could easily be adapted to such a system. The present 'hard wired' system has proved to be reliable; in one case a building was monitored for nine weeks and the apparatus operated continuously, without malfunctioning, throughout that period.

6. REFERENCES

- Condon, P.E., Grimsrud, D.T., Sherman, M.H. and Kammerud, R.C. (1980). An automated controlled-flow air infiltration measurement system. Building Air Change Rate and Infiltration Measurements, ASTM STP719. (ASTM 1980) pp60-72.
- Grot, R.A., Hunt, C.M. and Harrje, D.T. (1980). Automated air infiltration measurements in large buildings. Proceedings, First AIC Conference, Windsor Great Park, UK. pp105-108.
- Grot, R.A., Burch, D.M., Silberstein, S. and Galowin, L.S. (1982). Measurement methods for evaluation of thermal integrity of building envelopes. US Department of Commerce NBSIR 82-2605.
- Kronvall, J. (1980). Airtightness - Measurements and measurement methods. D8:1980 Swedish Council for Building Research, Sweden.
- Kumar, R., Ireson, A.D. and Orr, H.W. (1980). An automated air infiltration measuring system using SF₆ tracer gas in constant concentration and decay methods. Proceedings, First AIC Conference, Windsor Great Park, UK 1980. pp73-85.
- National Energy Advisory Committee (1980). Energy conservation in buildings. NEAC Report No.13.
- National Institute for Occupational Safety and Health (1977). Criteria for a recommended standard. Occupational Exposure to Waste Anaesthetic Gases and Vapours. Department of Health, Education and Welfare (National Institute for Occupation, Safety and Health) Publication No. 77-140.

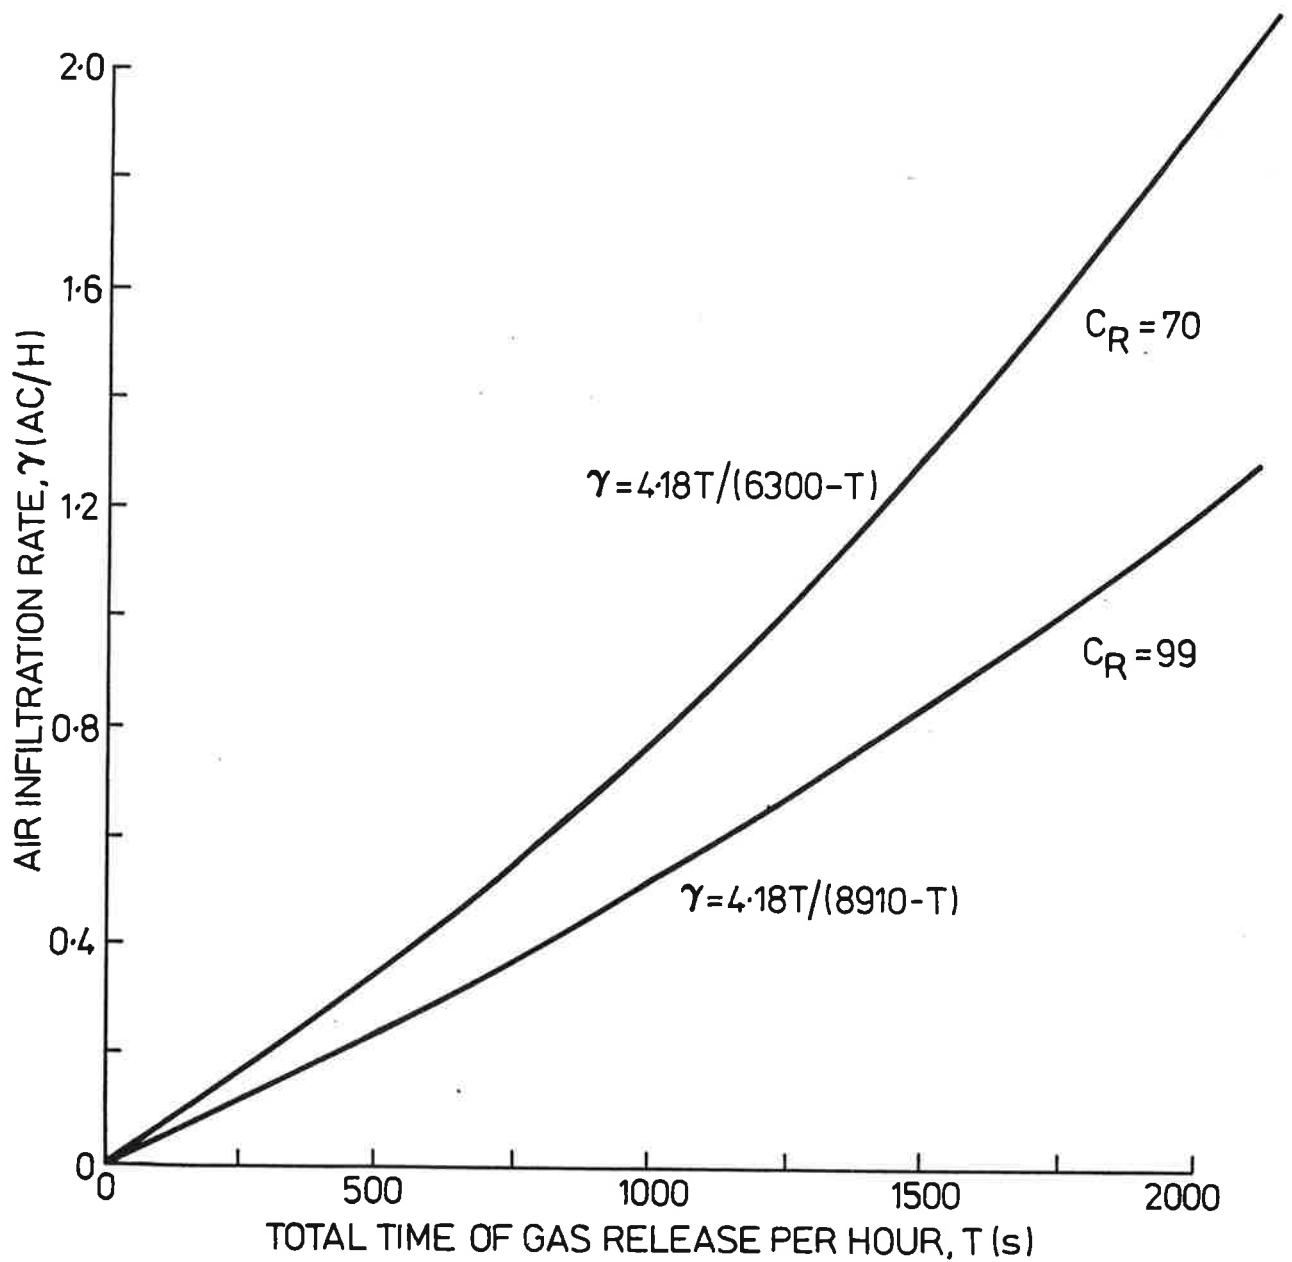


Figure 1. Air infiltration rate calculated as a function of the total time of gas release per hour, for two values of the reference concentration, C_R (ppm).

No. of release and sampling points = 6.

No. of gas releases per hour = 15 per location.

Gas flowrate $q = 11.6$ mL/s.

House volume = 250 m^3 .


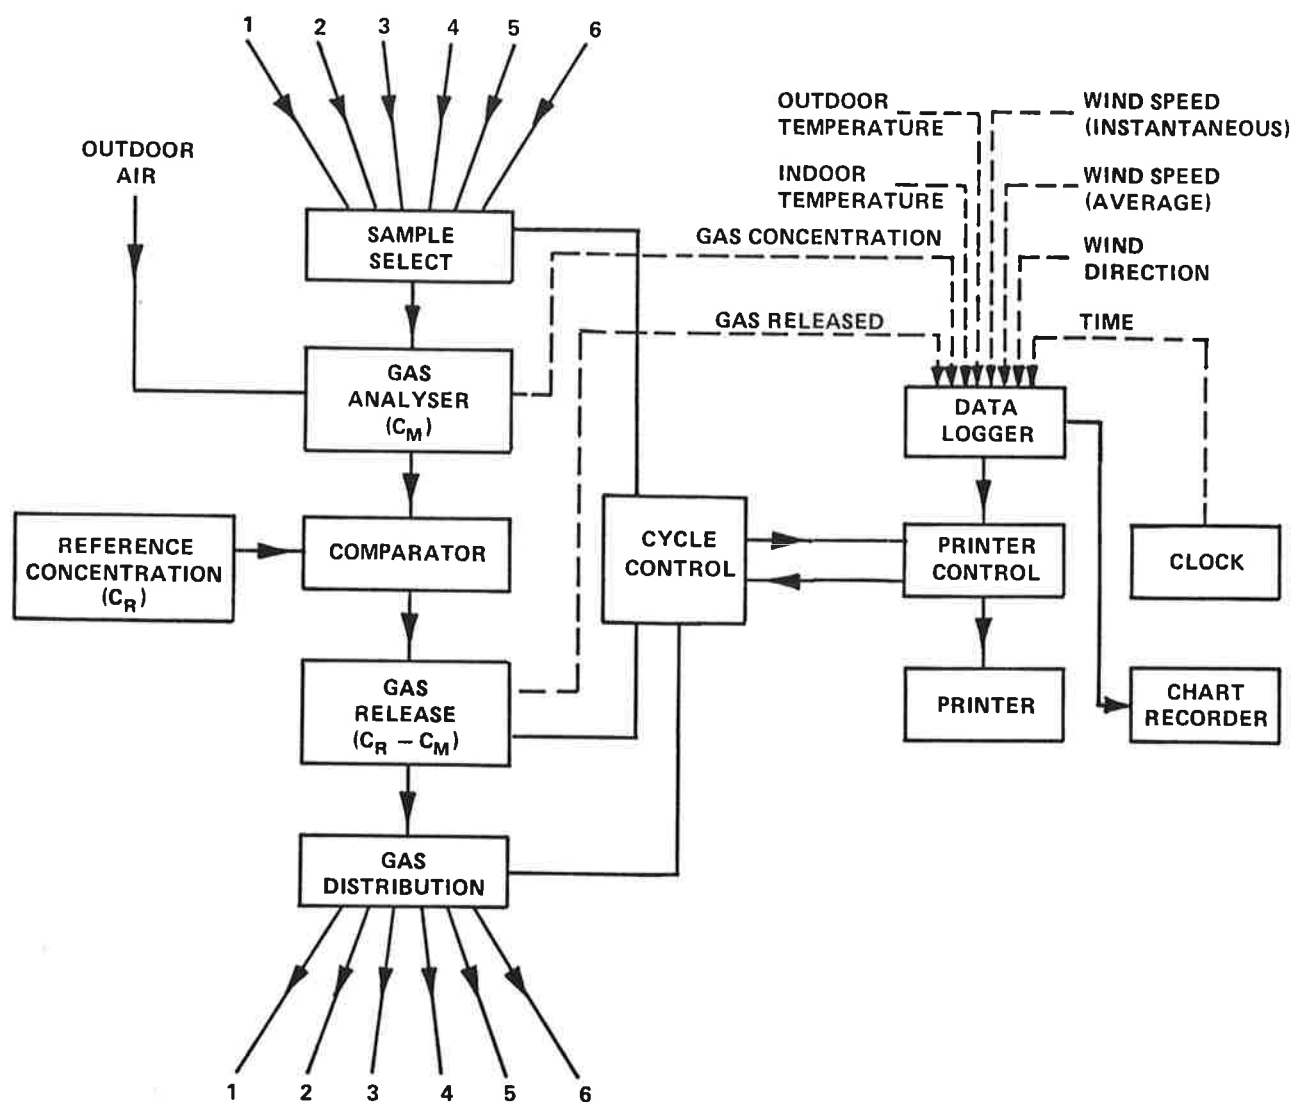


Figure 2. Block diagram of apparatus for continuous monitoring of air infiltration.

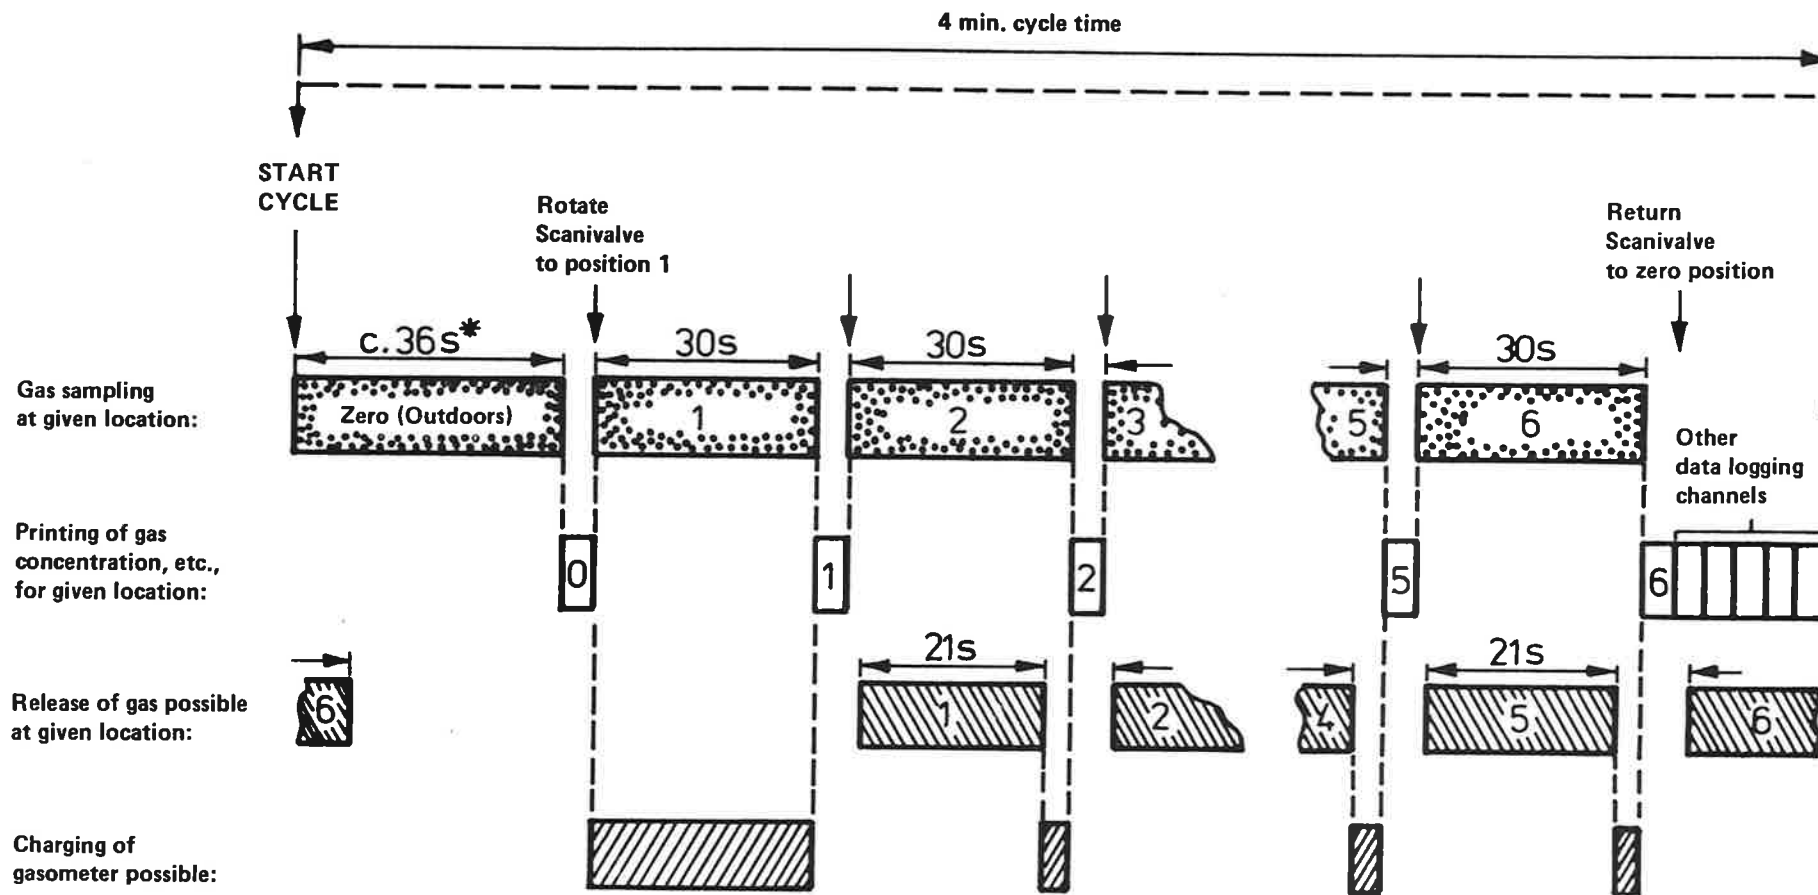

*Adjusted to give total cycle time of exactly 4 min.

Figure 3. Sequence diagram of the operations of the apparatus.

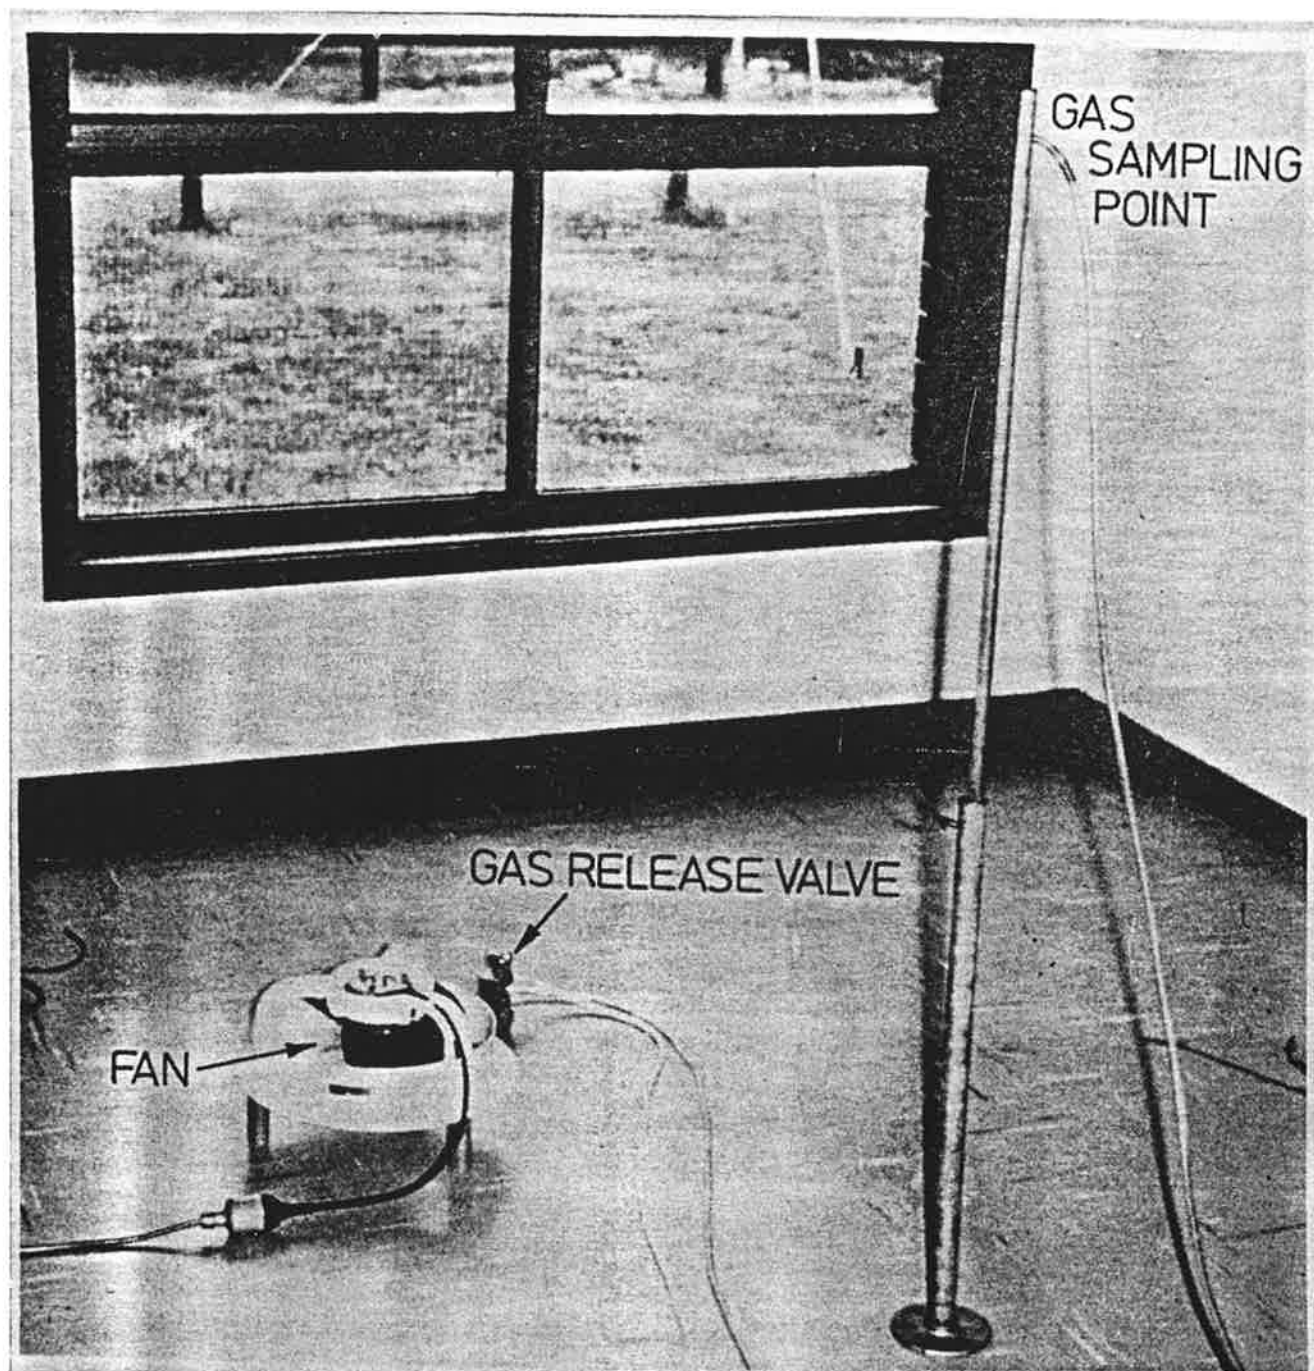


Figure 4. Typical arrangement of gas distribution fan and gas sampling tube in a room being monitored for air infiltration rate.

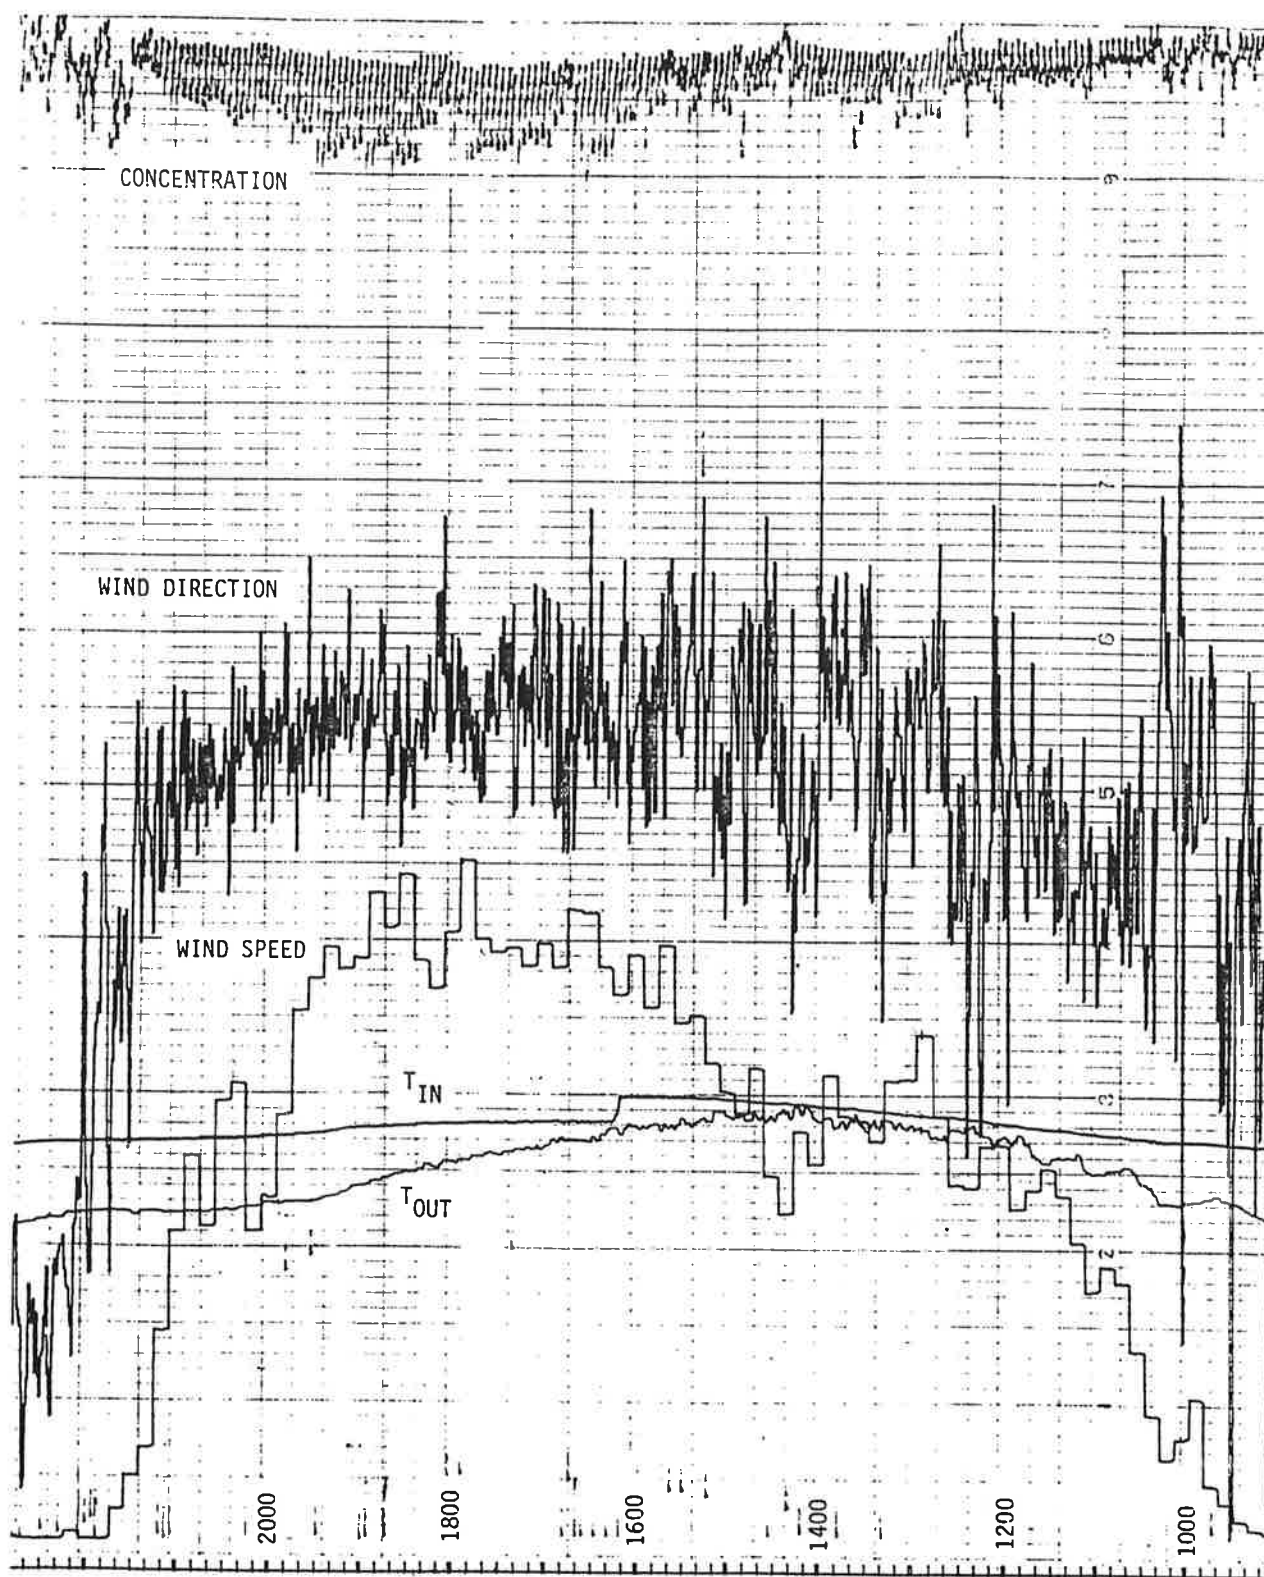


Figure 5. Chart recorder traces of gas concentration (100 ppm full scale deflection (FSD)), two-minute average values of wind speed (10 m/s FSD), wind direction sampled at one minute intervals (10 V FSD, 1 V equivalent to 45°), and indoor and outdoor temperatures (100°C FSD). Reference concentration 99 ppm.

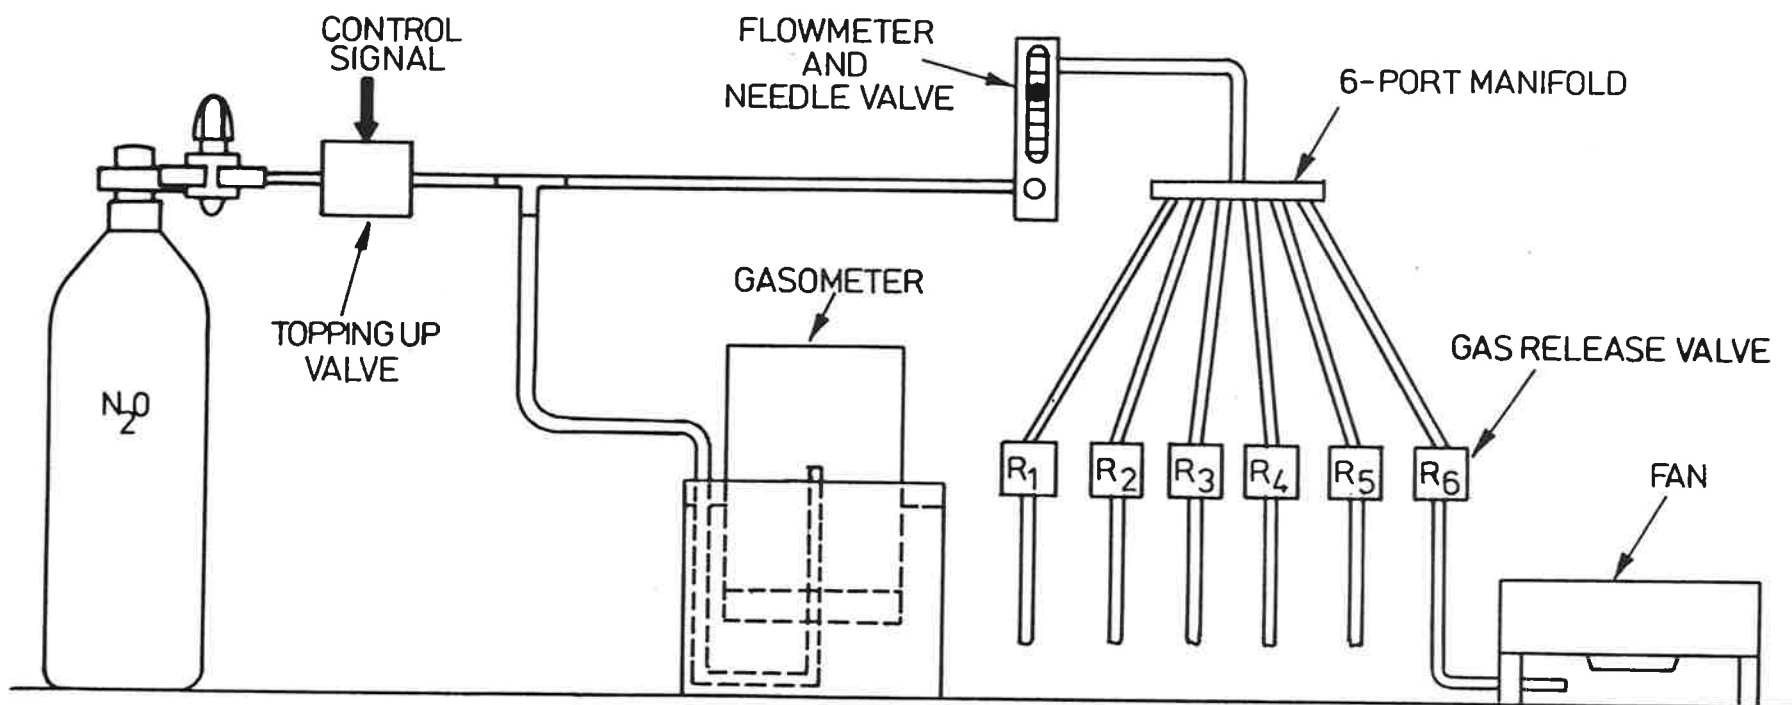


Figure 6. Schematic diagram of the apparatus for delivering tracer gas at a constant flowrate when a gas release valve is opened.

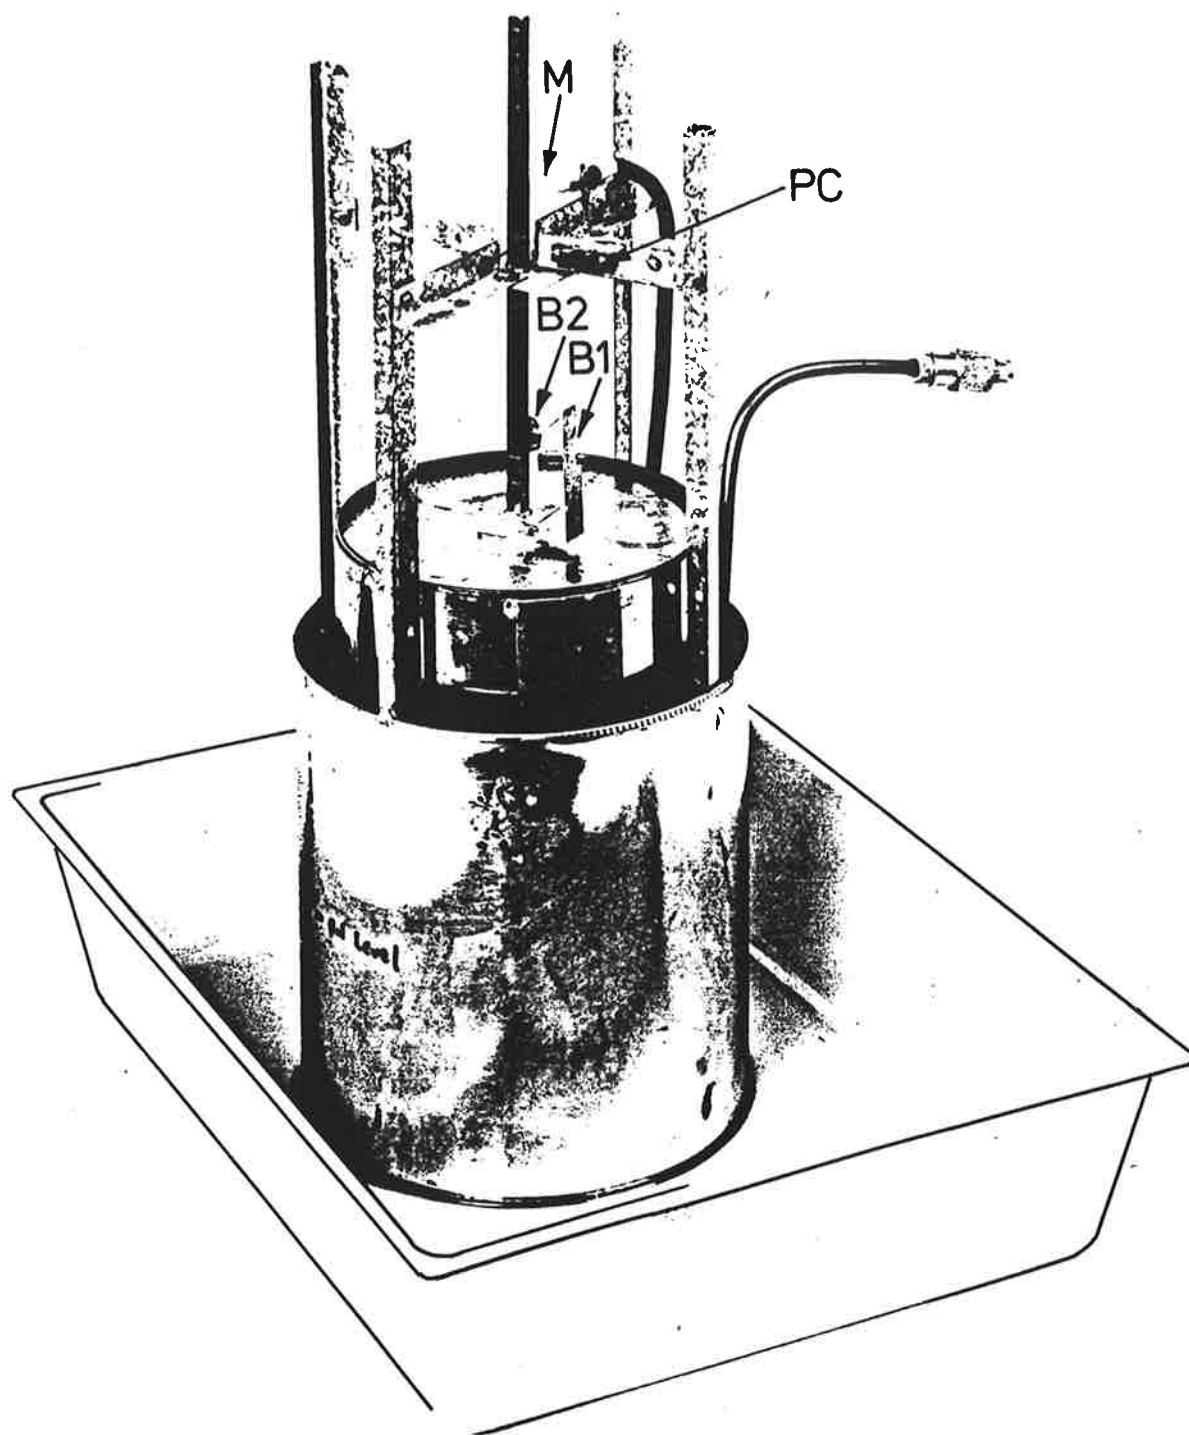


Figure 7. The gasometer used to supply tracer gas at constant pressure.

PC = infra-red 'photo-cell'.
B1 = blade to interrupt PC beam.
M = microswitch.
B2 = blade to trip M.